
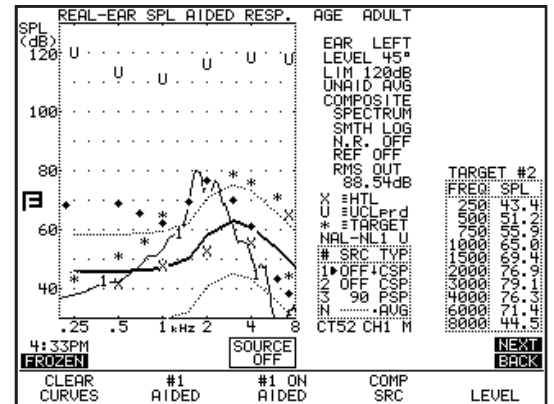



NEW!

FP35 v4.0

The FP35 Hearing Aid Analyzer is getting better than ever with the new release of software version 4.0. This release includes an improved new interface with simplified menus and a cleaner display for those who choose EASY rather than ADVANCED as their MENU choice.

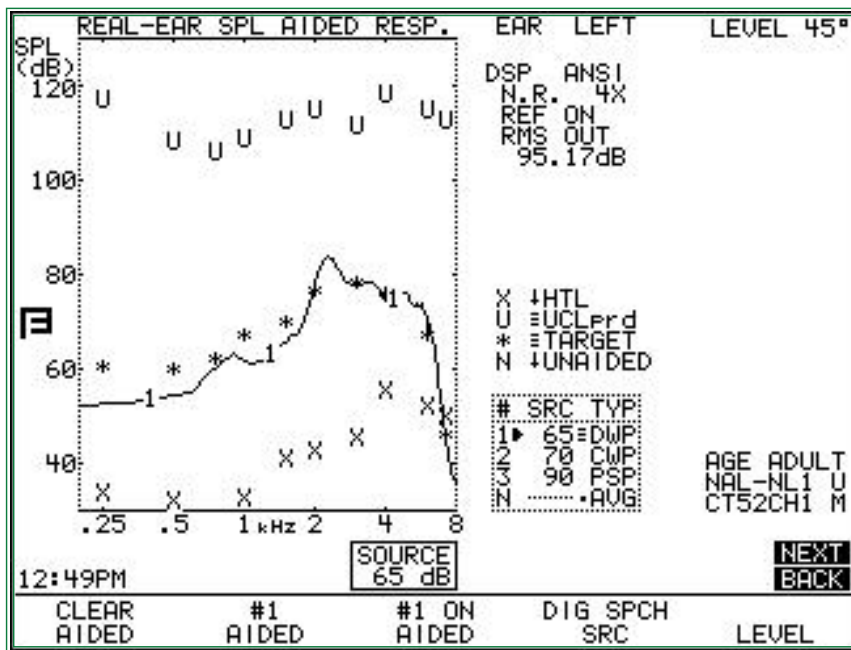

Also included is an Auto Stop feature that runs real-time measurements such as Digital Speech and Composite curves for a set amount of time, eliminating the need for the clinician to stop the measurement manually.

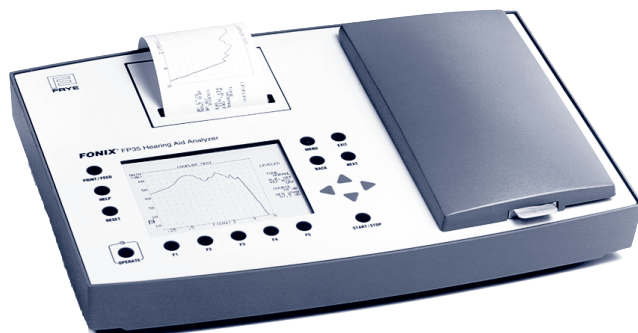

Version 4.0 was released on May 12, 2008. Units can be upgraded. Contact sales@frye.com for information.



FRYE ELECTRONICS, INC.

P.O. Box 23391 • Tigard, OR 97281-3391 • USA

(503) 620-2722 • (800) 547-8209

Fax: (503) 639-0128

www.frye.com • email: sales@frye.com